





www.nausicaa-medical.com

This medical device is intended for patient holding & positioning. It is not a restraint system. Before each use, it is important to check: the presence of the label, the stitches of the straps: that they do not fray or break, that the device does not show tears, snags, holes or signs of fraying (fabric and straps), that the buckles are not cracked or have no weak fastening.



FOR ALL CHAIRS




TO BE USED ONLY FOR THE INDICATED USE : TO PREVENT FROM FALLING



Maximal strap length : + 164 cm Belt height : + 11 cm Buckle : 50 mm

Simple and one size fits all, it is designed for different chair uses. Maximum useful area: 164 cm Without size constraints

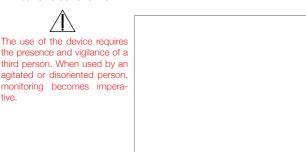

This medical device must be handled only by employees trained (by a healthcare professional) and qualified for its use (intended purpose, installation

and environment of use, etc.). If the medical device is incorrectly installed, there is a risk of accident for the patient.



v 07.02/25



CCMED2HP-PF



CE

Important Recommandations :

• In order to get a maximum efficiency of these sort of product,



- to choose the appropriate size for the patient
- to get the best possible adjustment to the patient
- These products must not be in direct contact with a wounded skin.



HOSPITAL RANGE Combination of polyurethan foam and on both faces Jersey/PU coating 100 % polyester bias 100 % polyester strap Nylon buckle

TO BE USED ONLY FOR THE INDICATED USE : TO PREVENT FROM FALLING

• Place the belt around the patient's abdomen (at hip level) and close the loop on the back of the chair.

